

# Acidic Protease Activity Colorimetric Microplate Assay Kit User Manual

Catalog # CAK1077

(Version 1.5E)

Detection and Quantification of Acidic Protease (ACP) Activity in Urine, Serum, Plasma, Tissue extracts, Cell lysate, Cell culture media and Other biological fluids Samples.

For research use only. Not for diagnostic or therapeutic procedures.



I. INTRODUCTION	2
II. KIT COMPONENTS	3
III. MATERIALS REQUIRED BUT NOT PROVIDED	4
IV. SAMPLE PREPARATION	4
V. ASSAY PROCEDURE	5
VI. CALCULATION	6
VII. TYPICAL DATA	7
VIII. TECHNICAL SUPPORT	7
IX NOTES	7



### I. INTRODUCTION

Acidic protease (ACP) can act on interior bond -C-NH- to hydrolyze the proteins of vegetable and animal in acid environment to form small peptides and amino acidics. The addition of this product to the processing of alcohol and distilled spirit can promote the growth of yeast to accelerate fermentation speed and improve alcohol productivity. In feedstuff industry, this product can be used as an additive by combined with other enzymes (such as cellulase, pectinase and  $\beta$ -glucanase, etc) for the preparation of complex feedstuff enzymes. It can further improve the nutrition value of feedstuff to accelerate the growth and increase the weight of livestock and poultry.

The assay is initiated with the enzymatic catalysis of casein by ACP in acid environment. The enzyme catalysed reaction products can be measured at a colorimetric readout at 660 nm.



# **II. KIT COMPONENTS**

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer	30 ml x 4	4 °C
Substrate	Powder x 1	4 °C
Stop Solution	12 ml x 1	4 °C
Reaction Buffer	6 ml x 1	4 °C
Dye Reagent	4 ml x 1	4 °C, keep in dark
Standard	Powder x 1	4 °C
Standard Diluent	5 ml x 1	4 °C
Positive Control	Powder x 1	4 °C
Plate Adhesive Strips	3 Strips	
Technical Manual	1 Manual	

# Note:

**Substrate**: add 4 ml Assay Buffer to dissolve before use.

Standard: add 1 ml Standard Diluent to dissolve before use, mix, heat at 50 °C water bath; then add 500  $\mu$ l into 500  $\mu$ l Standard Diluent, the concentration will be 5 mmol/L.

Positive Control: add 100 µl Assay Buffer to dissolve before use.



# III. MATERIALS REQUIRED BUT NOT PROVIDED

- 1. Microplate reader to read absorbance at 660 nm
- 2. Distilled water
- 3. Pipettor, multi-channel pipettor
- 4. Pipette tips
- 5. Mortar
- 6. Centrifuge
- 7. Timer
- 8. Ice

### IV. SAMPLE PREPARATION

# 1. For cell and bacteria samples

Collect cell or bacteria into centrifuge tube, discard the supernatant after centrifugation, add 1 ml Assay buffer for  $5 \times 10^6$  cell or bacteria, sonicate (with power 20%, sonicate 3s, interval 10s, repeat 30 times); centrifuged at 8000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

### 2. For tissue samples

Weigh out 0.1 g tissue, homogenize with 1 ml Assay buffer on ice, centrifuged at 8000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

For serum or plasma samplesDetect directly.



### V. ASSAY PROCEDURE

Add following reagents into the microcentrifuge tubes:

Reagent	Sample	Control	Positive	Standard	Blank		
			Control				
Sample	40 μΙ						
Positive Control			40 μΙ				
Standard				40 μΙ			
Standard Diluent					40 μΙ		
Assay Buffer		40 μΙ		40 μΙ	40 μΙ		
Substrate	40 μΙ	40 μΙ	40 μΙ				
Mix, put it in the oven, 40 °C for 15 minutes.							
Stop Solution	120 μΙ	120 μΙ	120 μΙ	120 μΙ	120 μΙ		
Mix, centrifuged at 10,000g 4 °C for 10 minutes, add the supernatant into the							
microplate.							
Supernatant	100 μΙ	100 μΙ	100 μΙ	100 μΙ	100 μΙ		
Reaction Buffer	60 μΙ	60 μΙ	60 μΙ	60 μΙ	60 μΙ		
Dye Reagent	40 μΙ	40 μΙ	40 μΙ	40 μΙ	40 μΙ		
Mix, incubate at room temperature for 20 minutes, measured at 660 nm and record							

Mix, incubate at room temperature for 20 minutes, measured at 660 nm and record the absorbance.

### Note:

- 1) Perform 2-fold serial dilutions of the top standards to make the standard curve.
- 2) For unknown samples, we recommend doing a pilot experiment & testing several doses to ensure the readings are within the standard curve range. If the enzyme activity is lower, please add more samples into the reaction system; or increase the reaction time; if the enzyme activity is higher, please dilute the sample, or decrease the reaction time.
- 3) If there is any precipitation or floc before read out, please centrifuged it in the microcentrifuge tubes at 4000g for 5 minutes, then add the supernatant into the plate, measured at 660 nm.
- 4) Reagents must be added step by step, can not be mixed and added together.



### VI. CALCULATION

**Unit Definition:** One unit of ACP activity is the enzyme that generates 1  $\mu$ mol of Tyrosine per minute.

1. According to the protein concentration of sample

ACP (U/mg) = 
$$(C_{Standard} \times V_{Standard}) \times (OD_{Sample} - OD_{Control}) / (OD_{Standard} - OD_{Blank}) / (V_{Sample} \times C_{Protein}) / T$$

$$= 0.333 \times (OD_{Sample} - OD_{Control}) / (OD_{Standard} - OD_{Blank}) / C_{Protein}$$

2. According to the weight of sample

ACP (U/g) = 
$$(C_{Standard} \times V_{Standard}) \times (OD_{Sample} - OD_{Control}) / (OD_{Standard} - OD_{Blank}) / (W \times V_{Sample} / V_{Assay}) / T$$

$$= 0.333 \times (OD_{Sample} - OD_{Control}) / (OD_{Standard} - OD_{Blank}) / W$$

3. According to the quantity of cells or bacteria

ACP (U/10<sup>4</sup>) = (
$$C_{Standard} \times V_{Standard}$$
) × (OD<sub>Sample</sub> - OD<sub>Control</sub>) / (OD<sub>Standard</sub> - OD<sub>Blank</sub>) / (N ×  $V_{Sample}$  /  $V_{Assay}$ ) / T = 0.333 × (OD<sub>Sample</sub> - OD<sub>Control</sub>) / (OD<sub>Standard</sub> - OD<sub>Blank</sub>) / N

4. According to the volume of serum or plasma

ACP (U/mI) = 
$$(C_{Standard} \times V_{Standard}) \times (OD_{Sample} - OD_{Control}) / (OD_{Standard} - OD_{Blank}) / V_{Sample} / T$$

$$= 0.333 \times (OD_{Sample} - OD_{Control}) / (OD_{Standard} - OD_{Blank})$$

C<sub>Protein</sub>: the protein concentration, mg/ml

W: the weight of sample, g

 $C_{Standard}$ : the concentration of Standard, 5 mmol/L = 5  $\mu$ mol/ml

N: the quantity of cell or bacteria,  $N \times 10^4$ 

V<sub>Sample</sub>: the volume of sample, 0.04 ml

V<sub>Standard</sub>: the volume of standard, 0.04 ml


V<sub>Assay</sub>: the volume of Assay buffer, 1 ml

T: the reaction time, 15 minutes




### VII. TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

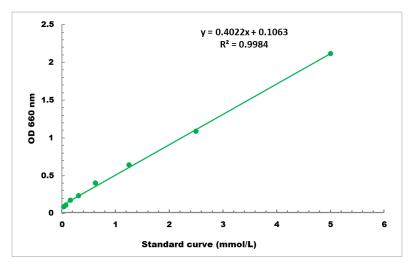

Detection Range: 0.05 mmol/L - 5 mmol/L

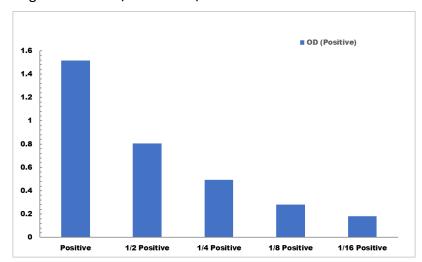

Positive Control reaction in 96-well plate assay with decreasing the concentration

### VIII. TECHNICAL SUPPORT

For troubleshooting, information or assistance, please go online to www.cohesionbio.com or contact us at techsupport@cohesionbio.com

# IX. NOTES