



Lactate Dehydrogenase Microplate Assay Kit User Manual

Catalog # CAK1007

(Version 2.3G)

Detection and Quantification of Lactate Dehydrogenase (LDH)
Activity in Urine, Serum, Plasma, Tissue extracts, Cell lysate, Cell
culture media and Other biological fluids Samples.

For research use only. Not for diagnostic or therapeutic procedures.

I. INTRODUCTION.....2

II. KIT COMPONENTS.....3

III. MATERIALS REQUIRED BUT NOT PROVIDED.....4

IV. SAMPLE PREPARATION.....4

V. ASSAY PROCEDURE.....5

VI. CALCULATION.....6

VII. TYPICAL DATA.....7

VIII. TECHNICAL SUPPORT.....7

IX. NOTES.....7

I. INTRODUCTION

Lactate dehydrogenase (LDH) is an oxidoreductase present in a wide variety of organisms. It catalyses the interconversion of pyruvate and lactate with concomitant interconversion of NADH and NAD. When disease or injury or toxic material damages tissues, cells release LDH into the bloodstream. Since LDH is a fairly stable enzyme, LDH has been widely used to evaluate the presence of damage and toxicity of tissue and cells. Quantification of LDH has broad range of applications.

Lactate Dehydrogenase Microplate Assay Kit provides a simple and direct procedure for measuring lactate dehydrogenase activity in a variety of samples. In this colorimetric LDH quantification assay, LDH reduces NAD to NADH, which then interacts with a specific probe to produce a color. The rate of increase in the absorbency at 450 nm, is a measure of LDH activity.

II. KIT COMPONENTS

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer	30 ml x 4	4 °C
Reaction Buffer	8 ml x 1	4 °C
Substrate	Powder x 1	-20 °C
Dye Reagent A	Powder x 1	4 °C
Dye Reagent B	1 ml x 1	4 °C
Standard	Powder x 1	4 °C
Positive Control	Powder x 1	-20 °C
Technical Manual	1 Manual	

Note:

Dye Reagent A: add 9 ml distilled water to dissolve before use, mix, store at 4°C.

Substrate: add 1 ml distilled water to dissolve before use, store at -20 °C.

Standard: add 1 ml distilled water to dissolve before use; then add 0.3 ml into 0.7 ml distilled water, the concentration will be 600 µmol/L.

Positive Control: add 0.1 ml distilled water to dissolve before use.

III. MATERIALS REQUIRED BUT NOT PROVIDED

1. Microplate reader to read absorbance at 450 nm
2. Distilled water
3. Pipettor, multi-channel pipettor
4. Pipette tips
5. Mortar
6. Ice
7. Centrifuge
8. Timer

IV. SAMPLE PREPARATION

1. For cell and bacteria samples

Collect cell or bacteria into centrifuge tube, discard the supernatant after centrifugation, add 1 ml Assay buffer for 5×10^6 cell or bacteria, sonicate (with power 20%, sonicate 3s, interval 10s, repeat 30 times); centrifuged at 8000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

2. For tissue samples

Weigh out 0.1 g tissue, homogenize with 1 ml Assay buffer on ice, centrifuged at 8000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

3. For serum or plasma samples

Detect directly.

V. ASSAY PROCEDURE

Add following reagents into the microplate:

Reagent	Sample	Control	Standard	Blank	Positive Control
Sample	10 μ l	--	--	--	--
Standard	--	--	100 μ l	--	--
Positive Control	--	--	--	--	10 μ l
Reaction Buffer	80 μ l	80 μ l	--	--	80 μ l
Substrate	10 μ l	10 μ l	--	--	10 μ l
Distilled water	--	10 μ l	--	100 μ l	--
Mix.					
Dye Reagent A	90 μ l	90 μ l	90 μ l	90 μ l	90 μ l
Dye Reagent B	10 μ l	10 μ l	10 μ l	10 μ l	10 μ l
Mix, incubate at room temperature for 5 minutes, record absorbance measured at 450 nm.					

Note:

- 1) Perform 2-fold serial dilutions of the top standards to make the standard curve.
- 2) For unknown samples, we recommend doing a pilot experiment & testing several doses to ensure the readings are within the standard curve range. If the enzyme activity is lower, please add more sample into the reaction system; or increase the reaction time; if the enzyme activity is higher, please dilute the sample, or decrease the reaction time.

VI. CALCULATION

Unit Definition: One unit of LDH activity is defined as the enzyme produce 1 nmol NADH per minute.

1. According to the volume of serum or plasma

$$\begin{aligned} \text{LDH (U/ml)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / V_{\text{Sample}} / T \\ &= 1200 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) \end{aligned}$$

2. According to the protein concentration of sample

$$\begin{aligned} \text{LDH (U/mg)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (V_{\text{Sample}} \\ &\quad \times C_{\text{Protein}}) / T \\ &= 1200 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / C_{\text{Protein}} \end{aligned}$$

3. According to the weight of sample

$$\begin{aligned} \text{LDH (U/g)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (W \times \\ &\quad V_{\text{Sample}} / V_{\text{Assay}}) / T \\ &= 1200 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / W \end{aligned}$$

4. According to the quantity of cell or bacteria

$$\begin{aligned} \text{LDH (U/10}^4) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (N \times \\ &\quad V_{\text{Sample}} / V_{\text{Assay}}) / T \\ &= 1200 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / N \end{aligned}$$

C_{Standard} : the concentration of standard, 600 $\mu\text{mol/L}$ = 600 nmol/ml;

C_{Protein} : the protein concentration, mg/ml;

W: the weight of sample, g;

V_{Sample} : the volume of sample, 0.01 ml;

V_{Standard} : the volume of standard, 0.1 ml;


V_{Assay} : the volume of Assay buffer, 1 ml;

T: the reaction time, 5 minutes;


N: the quantity of cell or bacteria, $N \times 10^4$.

VII. TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

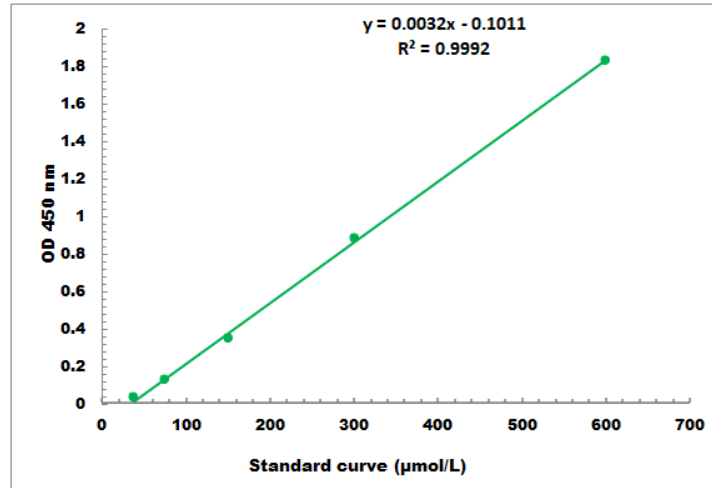

Detection Range: 30 µmol/L - 600 µmol/L

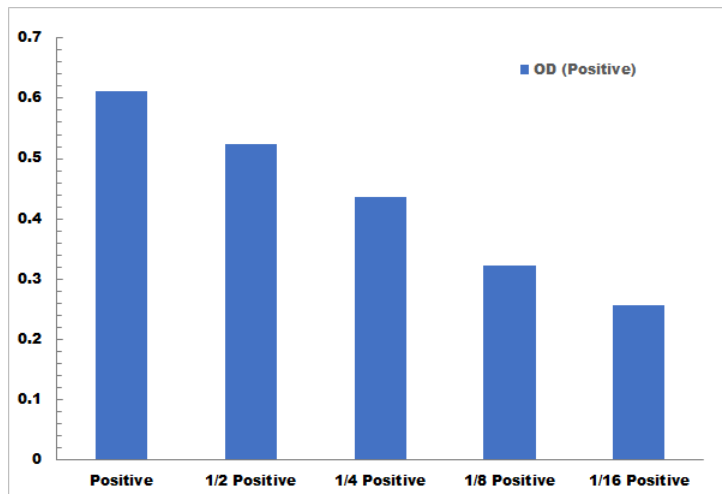

Positive Control reaction in 96-well plate assay with decreasing the concentration

VIII. TECHNICAL SUPPORT

For troubleshooting, information or assistance, please go online to www.cohesionbio.com or contact us at techsupport@cohesionbio.com

IX. NOTES