



# **Succinate Dehydrogenase (Mitochondrial Complex II) Microplate Assay Kit User Manual**

**Catalog # CAK1070**

(Version 1.5E)

Detection and Quantification of Succinate Dehydrogenase  
(Mitochondrial Complex II) Activity in Urine, Serum, Plasma, Tissue  
extracts, Cell lysate, Cell culture media and Other biological fluids  
Samples.

**For research use only. Not for diagnostic or therapeutic procedures.**

I. INTRODUCTION.....	2
II. KIT COMPONENTS.....	3
III. MATERIALS REQUIRED BUT NOT PROVIDED.....	4
IV. SAMPLE PREPARATION.....	4
V. ASSAY PROCEDURE.....	5
VI. CALCULATION.....	6
VII. TYPICAL DATA.....	7
VIII. TECHNICAL SUPPORT.....	7
IX. NOTES.....	7

## I. INTRODUCTION

Succinate Dehydrogenase (SDH) (EC 1.3.5.1) or succinate-coenzyme Q reductase (SQR) or respiratory complex II is an enzyme complex, which is bound to the inner mitochondrial membrane. SDH participates in both the citric acid cycle and electron transport chain. In mammals and many bacteria, SDH consists of 2 hydrophilic subunits, SDHA (flavoprotein) and SDHB (iron-sulfur protein) and 2 hydrophobic membrane anchor subunits: SDHC and SDHD. SDH oxidizes succinate to fumarate and transfers the electrons to ubiquinone. SDH deficiency in humans leads to a variety of phenotypes including Leigh syndrome, a neurometabolic disorder, tumor formation, and myopathy. Recent studies show that SDH can prevent the generation of ROS (reactive oxygen species); therefore, measurement of succinate dehydrogenase activity has wide applications.

Succinate Dehydrogenase Activity Microplate Assay Kit provides a simple and direct procedure for measuring succinate dehydrogenase activity levels in a variety of samples. The assay is initiated with the enzymatic hydrolysis of Succinic acid by SDH. The enzyme catalysed reaction products can be measured at a colorimetric readout at 450 nm.

## II. KIT COMPONENTS

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer I	30 ml x 4	4 °C
Assay Buffer II	1.2 ml x 1	4 °C
Assay Buffer III	20 ml x 1	4 °C
Substrate Dilution	10 ml x 1	4 °C
Substrate	Powder x 1	4 °C
Dye Reagent A	Powder x 1	4 °C
Dye Reagent B	1 ml x 1	4 °C
Standard	Powder x 1	-20 °C
Technical Manual	1 Manual	

### Note:

**Substrate:** add 9 ml Substrate Dilution to dissolve before use.

**Dye Reagent A:** add 9 ml distilled water to dissolve before use, mix, store at 4°C.

**Standard:** add 1 ml distilled water to dissolve before use; then add 0.3 ml into 0.7 ml distilled water, the concentration will be 600 µmol/L.

### **III. MATERIALS REQUIRED BUT NOT PROVIDED**

1. Microplate reader to read absorbance at 450 nm
2. Distilled water
3. Pipettor, multi-channel pipettor
4. Pipette tips
5. Mortar
6. Centrifuge
7. Timer
8. Ice

### **IV. SAMPLE PREPARATION**

1. For cell and bacteria samples

Collect cell or bacteria into centrifuge tube, discard the supernatant after centrifugation, add 0.99 ml Assay Buffer I and 10  $\mu$ l Assay Buffer II on ice, 10000g 4 °C for 10 minutes, discard the supernatant. Add 198  $\mu$ l Assay Buffer III and 2  $\mu$ l Assay Buffer II to the precipitation, shock, sonicate (with power 20%, sonicate 3s, interval 10s, repeat 30 times). Then add 800  $\mu$ l distilled water, mix, centrifuged at 10000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

2. For tissue samples

Weigh out 0.1 g tissue, homogenize with 0.99 ml Assay Buffer I and 10  $\mu$ l Assay Buffer II on ice, 10000g 4 °C for 10 minutes, discard the supernatant. Add 198  $\mu$ l Assay Buffer III and 2  $\mu$ l Assay Buffer II to the precipitation, shock, sonicate (with power 20%, sonicate 3s, interval 10s, repeat 30 times). Then add 800  $\mu$ l distilled water, mix, centrifuged at 10000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

## V. ASSAY PROCEDURE

Warm all reagents to room temperature before use.

Add following reagents into the microplate:

Reagent	Sample	Blank	Standard
Sample	10 $\mu$ l	--	--
Substrate	90 $\mu$ l	--	--
Standard	--	--	100 $\mu$ l
Distilled water	--	100 $\mu$ l	--
Dye Reagent A	90 $\mu$ l	90 $\mu$ l	90 $\mu$ l
Dye Reagent B	10 $\mu$ l	10 $\mu$ l	10 $\mu$ l
Mix, incubate at 37 °C for 2 minutes, measured at 450 nm and record the absorbance.			

### Note:

- 1) Perform 2-fold serial dilutions of the top standards to make the standard curve.
- 2) For unknown samples, we recommend doing a pilot experiment & testing several doses to ensure the readings are within the standard curve range. If the enzyme activity is lower, please add more sample into the reaction system; or increase the reaction time; if the enzyme activity is higher, please dilute the sample, or decrease the reaction time.
- 3) Reagents must be added step by step, can not be mixed and added together.

## VI. CALCULATION

**Unit Definition:** One unit of SDH activity is defined as the enzyme produce 1  $\mu\text{mol}$  NADH per minute.

### 1. According to the protein concentration of sample

$$\begin{aligned}\text{SDH (U/mg)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (V_{\text{Sample}} \\ &\quad \times C_{\text{Protein}}) / T \\ &= 3 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / C_{\text{Protein}}\end{aligned}$$

### 2. According to the weight of sample

$$\begin{aligned}\text{SDH (U/g)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (V_{\text{Sample}} \times \\ &\quad W / V_{\text{Assay}}) / T \\ &= 3 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / W\end{aligned}$$

### 3. According to the quantity of cells or bacteria

$$\begin{aligned}\text{SDH (U/10}^4\text{)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (V_{\text{Sample}} \\ &\quad \times N / V_{\text{Assay}}) / T \\ &= 3 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / N\end{aligned}$$

### 4. According to the volume of serum or plasma

$$\begin{aligned}\text{SDH (U/ml)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / V_{\text{Sample}} / T \\ &= 3 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / \text{OD}_{\text{Standard}}\end{aligned}$$

$C_{\text{Standard}}$ : the standard concentration, 600  $\mu\text{mol/L}$  = 0.6  $\mu\text{mol/ml}$ ;

$V_{\text{Standard}}$ : the volume of standard, 100  $\mu\text{l}$  = 0.1 ml;

$C_{\text{Protein}}$ : the protein concentration, mg/ml;

W: the weight of sample, g;

N: the quantity of cell or bacteria,  $N \times 10^4$ ;


$V_{\text{Sample}}$ : the volume of sample, 0.01 ml;

$V_{\text{Assay}}$ : the volume of Assay buffer, 1 ml;

T: the reaction time, 2 minutes.

## VII. TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

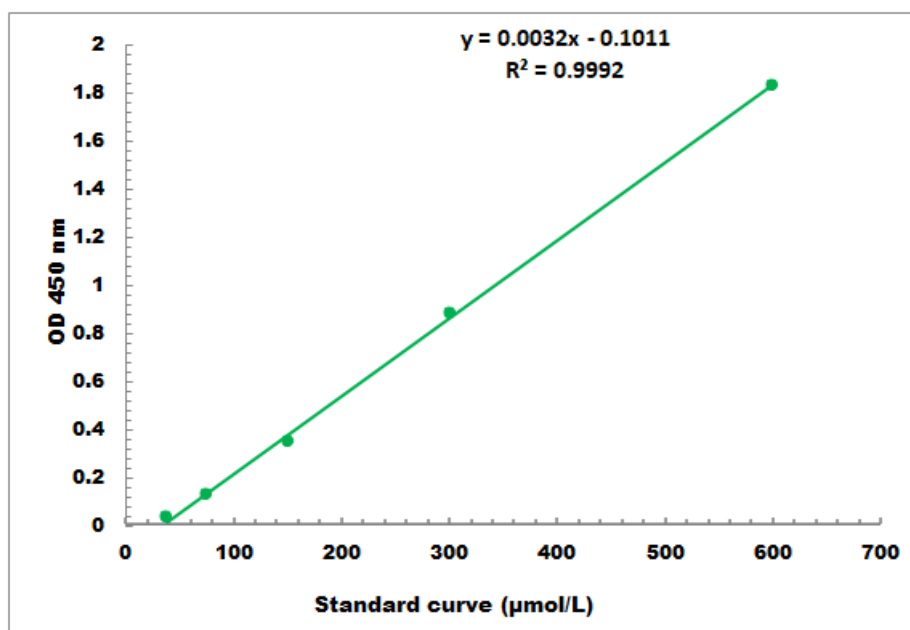

Detection Range: 30 μmol/L - 600 μmol/L

## VIII. TECHNICAL SUPPORT

For troubleshooting, information or assistance, please go online to [www.cohesionbio.com](http://www.cohesionbio.com) or contact us at [techsupport@cohesionbio.com](mailto:techsupport@cohesionbio.com)

## IX. NOTES