



# **Nitrite Microplate Assay Kit**

## **User Manual**

**Catalog # CAK1194**

(Version 1.2A)

Detection and Quantification of Nitrite Content in Serum, Plasma,  
Urine, Tissue extracts, Cell lysate, Cell culture media, Other  
biological fluids Samples.

**For research use only. Not for diagnostic or therapeutic procedures.**

I. INTRODUCTION.....	2
II. KIT COMPONENTS.....	3
III. MATERIALS REQUIRED BUT NOT PROVIDED.....	3
IV. SAMPLE PREPARATION.....	4
V. ASSAY PROCEDURE.....	5
VI. CALCULATION.....	6
VII. TYPICAL DATA.....	7
VIII. TECHNICAL SUPPORT.....	7
IX. NOTES.....	7

## I. INTRODUCTION

Nitrogen-based ions, nitrite and nitrate, are found in almost every living organism. Furthermore, endogenous Nitrite levels are found in mammals and also can be obtained from dietary sources. In humans, nitrite is further metabolized to Nitric Oxide and other reactive nitrogen species (nitrogen oxides). The Nitrate-Nitrite-NO biochemical pathway is well known for its participation in cell signaling, hypoxia-dependent response and regulation of blood flow. Recent studies suggest the reduction of Nitrite to Nitrogen Oxygen in the mitochondria. Specifically, myoglobin and xanthine oxidoreductase could generate NO under hypoxic conditions leading to mitochondrial respiration.

Nitrite Microplate Assay Kit utilizes the Griess Reagent, a classic protocol for the estimation of nitrite. In the assay, nitrite is reduced to Nitrogen Oxide using Griess Reagent I. Then, Nitrogen Oxide reacts with Griess Reagent II forming a stable product that can be detected by its absorbance at OD 540 nm.

## II. KIT COMPONENTS

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer I	30 ml x 1	4 °C
Assay Buffer II	30 ml x 1	4 °C
Dye Reagent Diluent	3 ml x 1	4 °C
Dye Reagent A	Powder x 1	4 °C
Dye Reagent B	Powder x 1	4 °C
Standard	Powder x 1	4 °C
Technical Manual	1 Manual	

### Note:

**Dye Reagent A:** add 2 ml Dye Reagent Diluent to dissolve before use.

**Dye Reagent B:** add 1 ml Dye Reagent Diluent to dissolve before use.

**Standard:** add 1 ml distilled water to dissolve before use, add 10 µl standard into 990 µl distilled water, mix; then add 1 µl diluted standard into 999 µl distilled water, mix; the concentration will be 1 nmol/ml.

## III. MATERIALS REQUIRED BUT NOT PROVIDED

1. Microplate reader to read absorbance at 540 nm
2. Distilled water
3. Pipettor, multi-channel pipettor
4. Pipette tips
5. Mortar
6. Centrifuge
7. Timer

#### **IV. SAMPLE PREPARATION**

##### **1. For tissue samples**

Weigh out 0.1 g tissue, homogenize with 0.5 ml distilled water, transfer all samples into centrifuge tube, add 0.25 ml Assay Buffer I, mix; then add 0.25 ml Assay Buffer II, mix; centrifuged at 10,000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube for detection.

##### **2. For liquid samples**

Add 0.5 ml samples into centrifuge tube, add 0.25 ml Assay Buffer I, mix; then add 0.25 ml Assay Buffer II, mix; centrifuged at 10,000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube for detection.

## V. ASSAY PROCEDURE

Add following reagents in the microplate:

Reagent	Sample	Standard	Blank
Sample	170 $\mu$ l	--	--
Standard	--	170 $\mu$ l	
Distilled water	--	--	170 $\mu$ l
Dye Reagent A	20 $\mu$ l	20 $\mu$ l	20 $\mu$ l
Mix well, incubate at room temperature for 3 minutes.			
Dye Reagent B	10 $\mu$ l	10 $\mu$ l	10 $\mu$ l
Mix, incubate at room temperature for 15 minutes, record absorbance measured at 540 nm.			

### Note:

- 1) Perform 2-fold serial dilutions of the top standards to make the standard curve.
- 2) The concentrations can vary over a wide range depending on the different samples.  
For unknown samples, we recommend doing a pilot experiment & testing several doses to ensure the readings are within the standard curve range.
- 3) Reagents must be added step by step, can not be mixed and added together.

## VI. CALCULATION

1. According to the weight of sample

$$\begin{aligned} \text{Nitrite (nmol/g)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (OD_{\text{Sample}} - OD_{\text{Blank}}) / (OD_{\text{Standard}} - OD_{\text{Blank}}) / (W \\ &\quad \times V_{\text{Sample}} / V_{\text{Assay}}) \\ &= (OD_{\text{Sample}} - OD_{\text{Blank}}) / (OD_{\text{Standard}} - OD_{\text{Blank}}) / W \end{aligned}$$

2. According to the volume of sample

$$\begin{aligned} \text{Nitrite (nmol/ml)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (OD_{\text{Sample}} - OD_{\text{Blank}}) / (OD_{\text{Standard}} - OD_{\text{Blank}}) / \\ &\quad V_{\text{Sample}} \times n \\ &= 2 \times (OD_{\text{Sample}} - OD_{\text{Blank}}) / (OD_{\text{Standard}} - OD_{\text{Blank}}) \end{aligned}$$

$C_{\text{Standard}}$ : the standard concentration, 1 nmol/ml;

$W$ : the weight of sample, g;

$V_{\text{Sample}}$ : the volume of sample, 0.17 ml;


$V_{\text{Standard}}$ : the volume of standard, 0.17 ml;

$V_{\text{Assay}}$ : the volume of distilled water and assay buffer, 1 ml;

$n$ : dilution factor,  $n=2$ .

## VII. TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

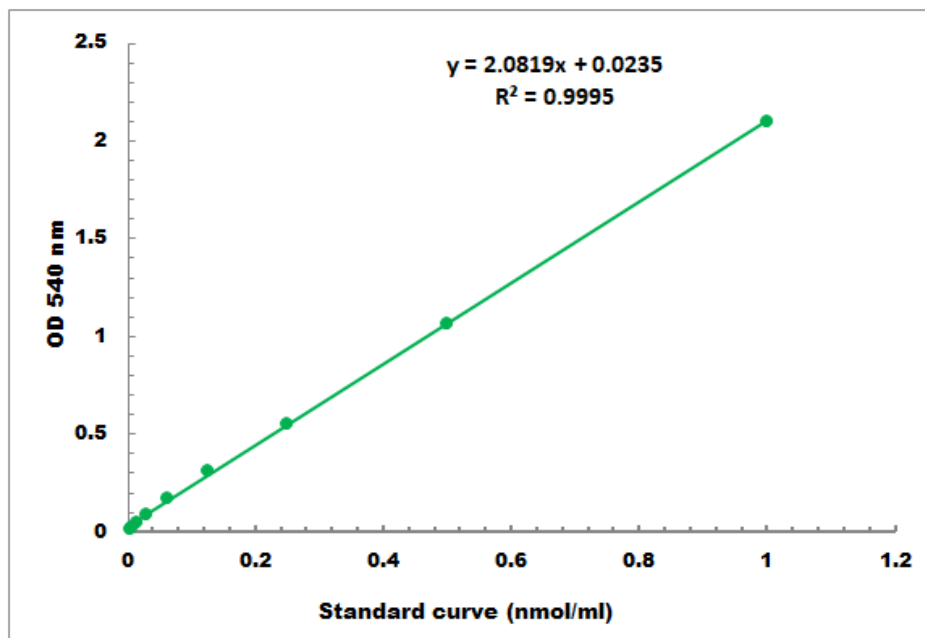

Detection Range: 0.01 nmol/ml - 1 nmol/ml

## VIII. TECHNICAL SUPPORT

For troubleshooting, information or assistance, please go online to [www.cohesionbio.com](http://www.cohesionbio.com) or contact us at [techsupport@cohesionbio.com](mailto:techsupport@cohesionbio.com)

## IX. NOTES