



Vitamin B9 ELISA Kit

User Manual

Catalog # CEK3081

(Version 1.1A)

Competitive Inhibition Enzyme Immunoassay for quantitative detection of Vitamin B9 concentrations in Serum, Plasma, Tissue Homogenates, Cell Lysates, Cell Culture Supernates or Other Biological Fluids.

For research use only. Not for diagnostic or therapeutic procedures.

I. INTRODUCTION.....	2
II. ASSAY PRINCIPLES.....	3
III. KIT COMPONENTS.....	4
IV. STORAGE AND STABILITY.....	4
V. MATERIALS REQUIRED BUT NOT PROVIDED.....	5
VI. HEALTH AND SAFETY PRECAUTIONS.....	5
VII. REAGENT PREPARATION.....	6
VIII. ASSAY PROCEDURE.....	9
IX. ASSAY PROCEDURE SUMMARY.....	11
X. TYPICAL DATA.....	12
XI. SENSITIVITY.....	12
XII. SPECIFICITY.....	12
XIII. CROSS REACTIVITY.....	13
XIV. TROUBLESHOOTING GUIDE.....	14
XV. TECHNICAL SUPPORT.....	15
XVI. NOTES.....	15

I. INTRODUCTION

Vitamin B9 (also called folate or Folic acid) belongs to one of the antioxidative water-soluble B vitamins. Vitamin B9 is an essential vitamin and human need to get it from the diet. It is naturally abundant in many foods but it is particularly enriched in dark green vegetables and liver. The main functions of folic acid are to synthesize nucleic acids and metabolize amino acids for cell division. Vitamin B9 is also suggested to be critical for promoting fertility and preventing heart diseases. Folate deficiency may cause diarrhea, depression, confusion, anemia, and fetal neural tube defects. The traditional techniques/instruments (HPLC or GC-MS) for detecting Vitamin B9 are complex, expensive, laborious, and time-consuming. Immunoassay techniques, such as ELISA, are commonly preferred as a simple, reliable and rapid methods.

II. ASSAY PRINCIPLES

Cohesion Biosciences Vitamin B9 ELISA Kit (Competitive Inhibition Enzyme Immunoassay) is a competitive inhibition enzyme immunoassay technique for the in vitro quantitative measurement of Vitamin B9 in Serum, Plasma, Tissue Homogenates, Cell Lysates, Cell Culture Supernates or Other Biological Fluids. This assay employs the competitive inhibition enzyme immunoassay technique. A monoclonal antibody specific to Vitamin B9 has been pre-coated onto a microplate. A competitive inhibition reaction is launched between biotin labeled Vitamin B9 and unlabeled Vitamin B9 (standards or samples) with the pre-coated antibody specific to Vitamin B9. After incubation the unbound conjugate is washed off. Next, Avidin conjugated to Horseradish Peroxidase (HRP) is added to each microplate well and incubated. The amount of bound HRP conjugate is reverse proportional to the concentration of Vitamin B9 in the sample. After addition of the substrate solution, the intensity of color developed is reverse proportional to the concentration of Vitamin B9 in the sample.

III. KIT COMPONENTS

Component	Volume
96-well Plate Pre-coated with Anti-Vitamin B9 Antibody	8 wells x 12 Strips
Vitamin B9 Standard	250 ng x 2
Biotin-Labeled Competitive Inhibitor (100X)	60 µl
Streptavidin-HRP (100X)	120 µl
Standard/Sample Diluent	30 ml
Biotin-Labeled Competitive Inhibitor Diluent	12 ml
Streptavidin-HRP Diluent	12 ml
Wash Buffer (20X)	30 ml
TMB Substrate Solution	12 ml
Stop Solution	12 ml
Plate Adhesive Strips	3 Strips
Technical Manual	1 Manual

IV. STORAGE AND STABILITY

All kit components are stable at 2 to 8 °C. Standard (recombinant protein) should be stored at -20 °C or -80 °C (recommended at -80 °C) after reconstitution. Opened Microplate Wells or reagents may be store for up to 1 month at 2 to 8 °C. Return unused wells to the pouch containing desiccant pack, reseal along entire edge.

Note: the kit can be used within one year if the whole kit is stored at -20 °C. Avoid repeated freeze-thaw cycles.

V. MATERIALS REQUIRED BUT NOT PROVIDED

1. Microplate reader capable of measuring absorbance at 450 nm.
2. Adjustable pipettes and pipette tips to deliver 2 µl to 1 ml volumes.
3. Adjustable 1-25 ml pipettes for reagent preparation.
4. 100 ml and 1 liter graduated cylinders.
5. Absorbent paper.
6. Distilled or deionized water.
7. Computer and software for ELISA data analysis.
8. Tubes to prepare standard or sample dilutions.

VI. HEALTH AND SAFETY PRECAUTIONS

1. Reagents provided in this kit may be harmful if ingested, inhaled or absorbed through the skin. Please carefully review the MSDS for each reagent before conducting the experiment.
2. Stop Solution contains 2 N Sulfuric Acid (H_2SO_4) and is an extremely corrosive agent. Please wear proper eye, hand and face protection when handling this material. When the experiment is finished, be sure to rinse the plate with copious amounts of running water to dilute the Stop Solution prior to disposing the plate.

VII. REAGENT PREPARATION

1. Sample Preparation

Store samples to be assayed within 24 hours at 2-8°C. For long-term storage, aliquot and freeze samples at -20°C. Avoid repeated freeze-thaw cycles.

Cell culture supernates: Remove particulates by centrifugation, assay immediately or aliquot and store samples at -20°C.

Serum: Allow the serum to clot in a serum separator tube (about 4 hours) at room temperature. Centrifuge at approximately 1000 X g for 15 minutes. Analyze the serum immediately or aliquot and store samples at -20°C.

Plasma: Collect plasma using heparin or EDTA as an anticoagulant. Centrifuge for 15 minutes at 1500 X g within 30 minutes of collection. Assay immediately or aliquot and store samples at -20°C.

Cell Lysates: Collect cells and rinse cells with PBS. Homogenize and lyse cells thoroughly in lysate solution. Centrifuge cell lysates at approximately 10000 X g for 5 minutes to remove debris. Aliquots of the cell lysates were removed and assayed.

Bone Tissue: Extract demineralized bone samples in 4 M Guanidine-HCl and protease inhibitors. Dissolve the final sample in 2 M Guanidine-HCl.

Tissue Homogenates: The preparation of tissue homogenates will vary depending upon tissue type. Rinse tissue with 1X PBS to remove excess blood, homogenized in 20 mL of 1X PBS and stored overnight at $\leq -20^{\circ}\text{C}$. After two freeze-thaw cycles were performed to break the cell membranes, the homogenates were centrifuged for 5 minutes at 5000 x g. The supernate was removed immediately and assayed.

Alternatively, aliquot and store samples at $\leq -20^{\circ}\text{C}$.

Note: Some lysis buffer, such as RIPA can not be used. Some components will affect the binding.

Urine: Urinary samples should be cleared by centrifugation and then can be used directly without dilution. Storage at -20°C.

2. Standard Preparation

Reconstitute the lyophilized Vitamin B9 Standard by adding 1 ml of Standard/Sample Diluent to make the 250 ng/ml standard stock solution. Allow solution to sit at room temperature for 5 minutes, then gently vortex to mix completely. Use within one hour of reconstituting. Two tubes of the standard (250 ng per tube) are included in each kit. Use one tube for each experiment.

Perform 2-fold serial dilutions of the top standards to make the standard curve within the range of this assay (3.9 ng/ml - 250 ng/ml) as below. Standard/Sample Dilution Buffer serves as the zero standard (0 ng/ml).

Standard	Add	Into
250 ng/ml		
125 ng/ml	500 µl of the Standard (250 ng/ml)	500 µl of the Standard/Sample Diluent
62.5 ng/ml	500 µl of the Standard (125 ng/ml)	500 µl of the Standard/Sample Diluent
31.2 ng/ml	500 µl of the Standard (62.5 ng/ml)	500 µl of the Standard/Sample Diluent
15.6 ng/ml	500 µl of the Standard (31.2 ng/ml)	500 µl of the Standard/Sample Diluent
7.8 ng/ml	500 µl of the Standard (15.6 ng/ml)	500 µl of the Standard/Sample Diluent
3.9 ng/ml	500 µl of the Standard (7.8 ng/ml)	500 µl of the Standard/Sample Diluent
0 ng/ml	1 ml of the Standard/Sample Diluent	

Note: The standard solutions are best used within 2 hours. The 250 ng/ml standard solution should be stored at 4°C for up to 12 hours, or at -20°C for up to 48 hours. Avoid repeated freeze-thaw cycles.

3. Biotin-Labeled Competitive Inhibitor Working Solution Preparation

The Biotin-Labeled Competitive Inhibitor should be diluted in 1:100 with the Biotin-Labeled Competitive Inhibitor Diluent and mixed thoroughly. The solution should be prepared no more than 2 hours prior to the experiment.

4. Streptavidin-HRP Working Solution Preparation

The Streptavidin-HRP should be diluted in 1:100 with the Streptavidin-HRP Diluent and mixed thoroughly. The solution should be prepared no more than 1 hour prior to the experiment.

5. Wash Buffer Working Solution Preparation

Pour entire contents (30 ml) of the Wash Buffer Concentrate into a clean 1,000 ml graduated cylinder. Bring final volume to 600 ml with glass-distilled or deionized water (1:20).

VIII. ASSAY PROCEDURE


The Streptavidin-HRP Working Solution and TMB Substrate Solution must be kept warm at 37°C for 30 minutes before use. When diluting samples and reagents, they must be mixed completely and evenly. Standard detection curve should be prepared for each experiment. The user will decide sample dilution fold by crude estimation of protein amount in samples.

1. Prepare 7 wells for standard, 1 well for blank. Add 50 μ l of each standard and samples into appropriate wells. Then add 50 μ l of Biotin-Labeled Competitive Inhibitor Working Solution to each well immediately.
2. Cover well and incubate for 60 minutes at room temperature with gentle shaking (using a microplate shaker is recommended).
3. Remove the cover, discard the solution and wash plate 3 times with Wash Buffer Working Solution, and each time let Wash Buffer Working Solution stay in the wells for 1 - 2 minutes. Blot the plate onto paper towels or other absorbent material. Do NOT let the wells completely dry at any time.
4. Add 100 μ l of Streptavidin-HRP Working Solution into each well and incubate the plate at 37°C for 45 minutes.
5. Wash plate 5 times with Wash Buffer Working Solution, and each time let wash buffer stay in the wells for 1 - 2 minutes. Discard the wash buffer and blot the plate onto paper towels or other absorbent material.
6. Add 100 μ l of TMB Substrate Solution into each well and incubate plate at 37°C in dark for 10 - 20 minutes.
7. Add 100 μ l of Stop Solution into each well. The color changes into yellow immediately.
8. Read the O.D. absorbance at 450nm in a microplate reader within 30 minutes after adding the Stop Solution.

For calculation, (the relative O.D.450) = (the O.D.450 of each well) - (the O.D.450 of Zero well). The standard curve can be plotted as the relative O.D.450 of each standard solution (Y) vs. the respective concentration of the standard solution (X). The concentration of the samples can be interpolated from the standard curve.


Note: If the samples measured were diluted, multiply the dilution factor to the concentrations from interpolation to obtain the concentration before dilution.

IX. ASSAY PROCEDURE SUMMARY

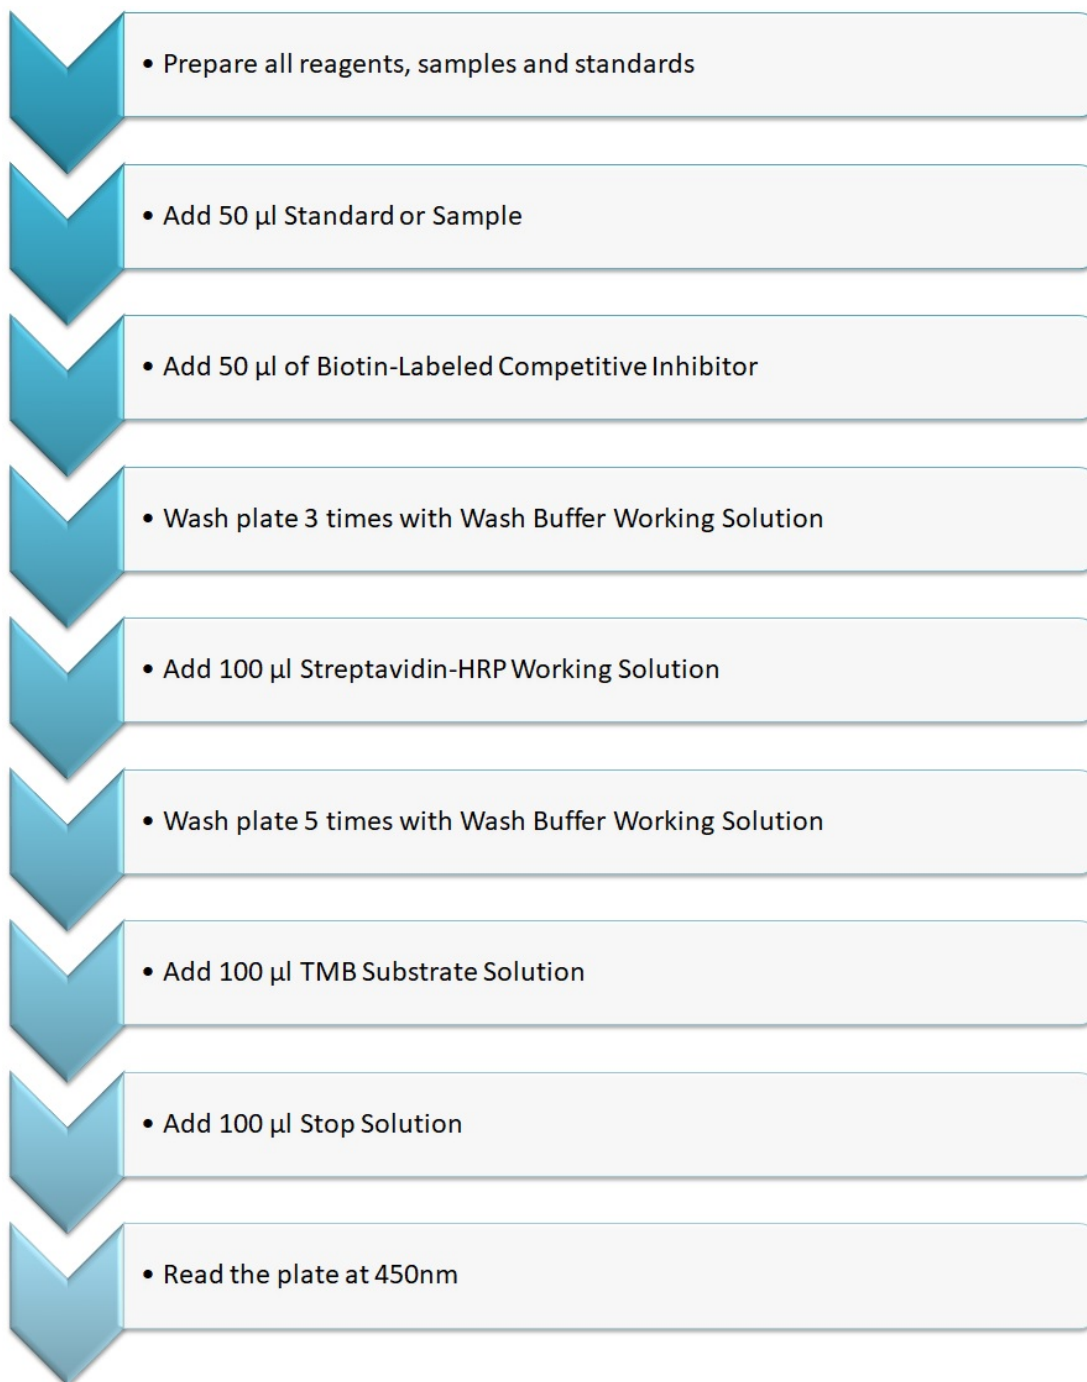

X. TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

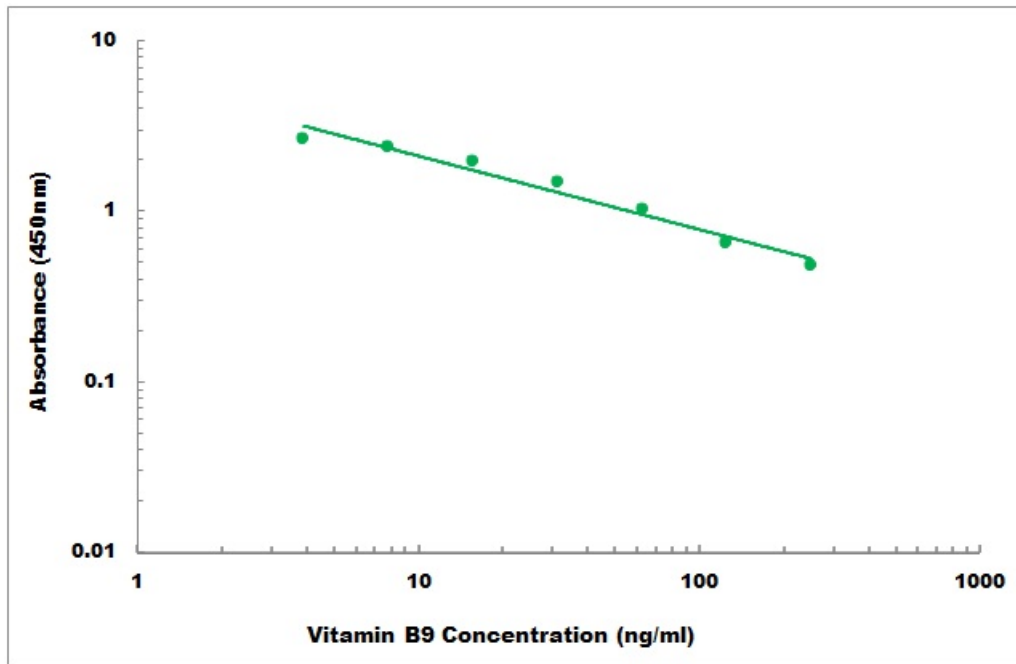

XI. SENSITIVITY

The minimum detectable dose of Vitamin B9 is typically less than 1.23 ng/ml.

XII. SPECIFICITY

Vitamin B9 ELISA Kit has high sensitivity and excellent specificity for detection of Vitamin B9.

The detection range is 3.9 ng/ml - 250 ng/ml.

XIII. CROSS REACTIVITY

No significant cross-reactivity or interference between Vitamin B9 and analogues was observed.

XIV. TROUBLESHOOTING GUIDE

Problem	Possible Cause	Solution
High signal and background in all wells	• Insufficient washing	• Increase number of washes • Increase time of soaking between in wash
	• Too much Streptavidin-HRP	• Check dilution, titration
	• Incubation time too long	• Reduce incubation time
	• Development time too long	• Decrease the incubation time before the stop solution is added
No signal	• Reagent added in incorrect order, or incorrectly prepared	• Review protocol
	• Standard has gone bad (If there is a signal in the sample wells)	• Check the condition of stored standard
	• Assay was conducted from an incorrect starting point	• Reagents allows to come to 20 - 30 °C before performing assay
Too much signal-whole plate turned uniformly blue	• Insufficient washing-unbound Streptavidin-HRP remaining	• Increase number of washes Carefully
	• Too much Streptavidin-HRP	• Check dilution
	• Plate sealer or reservoir reused, resulting in presence of residual Streptavidin-HRP	• Use fresh plate sealer and reagent reservoir for each step
Standard curve achieved but poor discrimination between point	• Plate not developed long enough	• Increase substrate solution incubation time
	• Improper calculation of standard curve dilution	• Check dilution, make new standard curve
No signal when a signal is expected, but standard curve looks fine	• Sample matrix is masking detection	• More diluted sample Recommended
Samples are reading too high, but standard curve is fine	• Samples contain protein levels above assay range	• Dilute samples and run Again
Edge effect	• Uneven temperature around work surface	• Avoid incubating plate in areas where environmental conditions vary • Use plate sealer

XV. TECHNICAL SUPPORT

For troubleshooting, information or assistance, please go online to www.cohesionbio.com or contact us at techsupport@cohesionbio.com

COHESION BIOSCIENCES LIMITED

FLAT32 ADVENTURES COURT

12 NEWPORT AVENUE

LONDON, E14 2DN, UK

Website: www.cohesionbio.com

Email: order@cohesionbio.com

techsupport@cohesionbio.com

custom@cohesionbio.com

XVI. NOTES